



Comparison of Central Corneal Thickness Measured by Standard Ultrasound Pachymetry, Corneal Topography, Tono-Pachymetry and Anterior Segment Optical Coherence Tomography

Javier González-Pérez, Juan Queiruga Piñeiro, Ángelx Sánchez García & José Manuel González Méijome

To cite this article: Javier González-Pérez, Juan Queiruga Piñeiro, Ángelx Sánchez García & José Manuel González Méijome (2018): Comparison of Central Corneal Thickness Measured by Standard Ultrasound Pachymetry, Corneal Topography, Tono-Pachymetry and Anterior Segment Optical Coherence Tomography, Current Eye Research, DOI: [10.1080/02713683.2018.1461910](https://doi.org/10.1080/02713683.2018.1461910)

To link to this article: <https://doi.org/10.1080/02713683.2018.1461910>



Accepted author version posted online: 10 Apr 2018.



Submit your article to this journal [↗](#)



Article views: 1



View related articles [↗](#)



View Crossmark data [↗](#)

Comparison of Central Corneal Thickness measured by Standard Ultrasound Pachymetry, Corneal Topography, Tono-Pachymetry and Anterior Segment Optical Coherence Tomography.

Javier González-Pérez, OD, PhD, FIACLE,¹ Juan Queiruga Piñeiro OD, MSc,^{1,2} Ángel Sánchez García OD, MSc,¹ José Manuel González Méijome OD,^{1,3} PhD, FIACLE.

¹ Ocular Surface and Contact Lens Research Laboratory. Faculty of Optometry. University of Santiago de Compostela, Spain.

² Instituto Oftalmológico Fernández-Vega, Oviedo, Spain.

³ Clinical & Experimental Optometry Research Lab. Center of Physics (Optometry) - School of Sciences. University of Minho, 4710-057 Gualtar – Braga, Portugal.

Running Head Title: Reliability of Ultrasound and 3 non-contact pachymeters

Corresponding Author:

Javier González-Pérez, OD, PhD
Lab. SOYLC – Applied Physics (Optometry)
Faculty of Optometry
University of Santiago de Compostela
15782 Santiago de Compostela (Spain)
Telephone: +34 881 813 537 / 881 813 504
e-mail: javier.gonzalez@usc.es

Key-words: Central corneal thickness, ultrasound pachymetry, non-contact tonopachymetry, Scheimpflug camera, anterior segment optical coherence tomography, interchangeability.

Acknowledgement and Disclosure:

The authors declare that they do not have any proprietary or financial interest in any of the materials mentioned in this article.

Abstract

Purpose: To compare central corneal thickness (CCT) measured by standard ultrasound pachymetry (USP), and three non-contact devices in healthy eyes.

Methods: A cross-sectional study of CCT measurement in 52 eyes of 52 healthy volunteers was done by a single examiner at Ocular Surface and Contact Lens Laboratory. Three consecutive measurements were done by standard USP, non-contact tonometer, Pentacam corneal topographer, and Anterior Segment Optical Coherence Tomography (AS-OCT). The mean values were used for assessment. The results were compared using **multivariate ANOVA**, linear regression and Pearson correlation. Agreement among the devices was analyzed using mean differences and Bland-Altman analysis with 95% limits of agreement (LoA). Finally, reliability was analyzed using intraclass correlation coefficient (ICC).

Results: Mean CCT by ultrasound pachymeter, tonometer, corneal topographer and AS-OCT were $558.9 \pm 31.2 \mu\text{m}$, $525.8 \pm 43.1 \mu\text{m}$, $550.4 \pm 30.5 \mu\text{m}$ and $545.9 \pm 30.5 \mu\text{m}$ respectively. There was a significant positive correlation between AS-OCT and USP (Pearson correlation = 0.957, $p < 0.001$), corneal topography and USP (Pearson correlation = 0.965, $p < 0.001$) and corneal topography and AS-OCT (Pearson correlation = 0.965, $p < 0.001$). There was a lower correlation between CT-1P tonometer and the other three modalities. Intraclass correlation coefficients show an excellent reliability between pairs except for CT-1P against the other three instruments that were found moderate.

Conclusions: CT-1P tonometer underestimates CCT measurements compared to Scheimpflug system, AS-OCT device, and USP. Mean CCT among USP, Pentacam and AS-OCT were comparable and had significant linear correlations. In clinical practice, these three modalities could be interchangeable in healthy patients.

Introduction

Central corneal thickness (CCT) is an important and sensitive indicator of corneal health.¹ It is necessary in monitoring corneal diseases such as corneal oedema, keratoconus, Fuchs dystrophy, glaucoma and to evaluate corneal barrier and endothelial pump function in several surgical conditions.²⁻⁴ In clinical practice, it is useful in the evaluation of contact lens wear,^{5,6} selecting patients for refractive surgery and posterior evaluation.^{7,8}

CCT is also a predictive factor for glaucoma progression in patients with high baseline intraocular pressure (IOP). Moreover, CCT is an important parameter in the risk profiling of ocular hypertensive to glaucoma patient.^{9,10} Since IOP measurement by applanation tonometry is influenced by CCT, it is important to obtain the reliable corneal pachymetry for each patient and adjust the IOP for the measured CCT.^{1,11}

There are numerous methods available to measure CCT. Ultrasound pachymetry (USP) has been widely considered as the gold standard because it is very easy, fast and convenient to repeat several measurements to minimize error.^{12,13} USP requires contact with the cornea and uses the Doppler Effect to determine CCT. Disadvantages of ultrasonic pachymetry include direct placement of the probe on the cornea, the risk infection and corneal epithelial damage, the necessity for topical anesthesia (which may influence by up to 10 microns CCT measurements), and dependence on examiner experience for reliable measurements.¹⁴⁻¹⁵

Optical Coherence Tomography (OCT), which was introduced in the early 1990s, is a noncontact imaging method that provides detailed cross-sectional images of biological tissues by measuring their optical reflections.^{16,17} OCT has been widely used clinically

in ophthalmologic practice for the last two decades.¹⁸⁻¹⁹ In recent years, OCT technology has experimented the incorporation of spectral-domain (SD) imaging that offers significant advantages over the traditional time-domain (TD) techniques, which include faster imaging speed, higher resolution, and better visualization.²⁰ Simultaneously with these improvements, the utility of OCT in the ophthalmic practice has become more extended. Particularly, anterior segment OCT (AS-OCT), which provides high-resolution cross-sectional images of anterior segment structures, including corneal thickness, anterior chamber angle, conjunctiva, and tear meniscus, has recently gained popularity.²¹⁻²⁴ There are very few studies giving comparative accuracy of CCT measurements by AS-OCT versus USP.^{4,25}

The Pentacam, developed in 2000s, uses a rotating Scheimpflug camera and a slit-light source that rotate together around the optical axes of the eye to calculate a three-dimensional model of the anterior segment. A total of 25 images are captured within 2 sg, with each slit image composed of 25,000 points including 500 true elevation points. As a pachymeter, Pentacam provides a corneal thickness map and determines the thinnest point as well. Previous studies have shown that Pentacam has high agreement compared with USP,¹² high intraoperator repeatability and reproducibility for CCT measurements.^{26,27}

In recent years, several units of non-contact tonometry and pachymetry have been developed. Tono-pachymetry simultaneously measures CCT using the principle of the Scheimpflug camera system and IOP using a conventional non-contact tonometry method. Tono-pachymetry is patient-friendly and time-saving, but it has not been well documented whether the CCT values obtained from tono-pachymetry are comparable to those derived from conventional USP as the gold standard for measuring CCT.^{28,29}

To the best knowledge of the authors, this was one of the few studies that was designed to compare the correlation and agreement between CCT measurements

obtained using recently marketed, CT-1P tonopachymetry, 3D OCT-2000 and Pentacam with USP in young myopic healthy eyes.

Materials and Methods

Study Design and subjects: This prospective cross-sectional comparative study includes 52 eyes of 52 healthy subjects voluntarily enrolled at the Ocular Surface and Contact Lens Laboratory (LSOYLC) from the University of Santiago de Compostela. All subjects after CCT measurement were subjected to a full ophthalmic examination. This examination included routine evaluation of visual acuity, refractive error and slit lamp biomicroscopy with particular attention to the presence of ocular adverse events. The inclusion criteria were age between 18-30 years, normal corneal topographic pattern, myopia between -6.00 D and -0.75 D, no more than -1.75 D of astigmatism, correctable to 20/20 and also included emmetropic eyes achieving 20/20 or better visual acuity. Exclusion criteria included previous refractive surgery, corneal diseases, recent use of contact lenses, no other systemic or ocular diseases, and use of topical medications.

The study was performed according to the renewed and revised rules of Helsinki Declaration and was approved by the Ethics Committee of the University of Santiago de Compostela.

Technologies used to measure CCT: Three consecutive measurements were done by standard USP, non-contact tonopachymeter, corneal topography, and anterior segment optical coherence tomography (AS-OCT). In order to eliminate effects of diurnal variation on thickness, all measurements were taken between 2 PM and 6 PM.³⁰

Automatic analysis by Scheimpflug camera Pentacam (Oculus Optikgerate GmbH, Wetzlar, Germany) was performed for all eyes. Multiple slit images of the anterior segment with 500 true elevation points are captured by the rotating camera. CCT was recorded only when the examination quality specification reading was satisfactory; otherwise it was excluded and reanalyzed until three valid readings were obtained.

Spectral-domain optical coherence tomographic 3D OCT-2000 (Topcon, Tokyo, Japan) equipment was used for anterior segment analysis using the headrest attachment. It captures high resolution images of the cornea using non-contact OCT, allowing for topographical mapping of the cornea including corneal thickness. The system obtained different images, separated by 0.25 mm with 5-6 micron of axial resolution and 20 microns of transverse resolution. The corneal thickness was measured by an automated algorithm, that detects epithelium and endothelium limits on the cross-sectional images of the cornea. The mean value from three consecutive measurements was taken as the CCT value.

The non-contact tonopachymeter CT-1P (Topcon, Tokyo, Japan), also was used for pachymetric analysis by a specular microscope method. The patient was seated and asked to look at a fixation target. The emitted light from a narrow slit in the cornea is reflected by the front and backside of the cornea and CCT was measured according to the interval between both reflection images on the line sensor. The operator visualized a real-time image of the patient's eye on the screen. Although the operator manually focused the image to the center of the pupil, CT-1P tonopachymeter automatically measured CCT three times and calculated the average value.

These non-contact measurements were followed by USP (Paxis, Biovision Inc, Clermont-Ferrand, France). The subject was seated on the chair and asked to look at fixation light located straight ahead. The examiner placed the pachymeter probe on the

central cornea as perpendicular as possible. Three consecutive measurements were taken by the same experienced examiner and the average was recorded for each patient. USP was performed under topical anesthesia with tetracaine hydrochloride 0,5% (Colircusí Anestésico, Alcon Cusí, Barcelona, Spain).

Data Analysis: Data were analyzed by SPSS version 20 (SPSS Inc., Chicago, Illinois, USA) using descriptive statistics, linear regression and Pearson correlation coefficient. The CCT measured by USP and the three non-contact devices was compared using **multivariate** analysis of variance (ANOVA), and pairwise comparisons were performed using the Bonferroni adjustment for multiple comparisons. A p-value of less than 0.05 was considered statistically significant. Bland-Altman plot was used to evaluate the agreement between the four techniques. Finally, reliability was analyzed using intraclass correlation coefficient (ICC). Based on the 95% confident interval of the ICC estimate, values less than 0.5, between 0.5 and 0.75, between 0.75 and 0.9, and greater than 0.90 are indicative of poor, moderate, good, and excellent reliability, respectively.³¹⁻³²

Results

A total of 52 eyes in 52 healthy subjects (only right eyes) were studied (32 females and 20 males). The mean age was 23.52 ± 3.78 years (range 20 to 28 years) and a mean spherical equivalent of -1.56 ± 1.78 D (range -0.50 to -5.75 D).

The highest CCT mean value was obtained with the USP (558.9 ± 31.2 μm ; range from 476 to 614 μm), followed by the Pentacam (550.4 ± 30.5 μm ; range from 465 to 615 μm), then by the 3D OCT (545.9 ± 30.5 μm ; range from 457 to 602 μm), and finally, the

lowest value was obtained with the tono-pachymeter ($525.8 \pm 43.1 \mu\text{m}$; range from 431 to $674 \mu\text{m}$).

Figure 1 shows a significant positive correlation between the CCT readings obtained by USP and by the non-contact devices. There was a significant strong correlation between AS-OCT and USP (Pearson correlation = 0.979, $p < 0.001$), Pentacam and USP (Pearson correlation = 0.946, $p < 0.001$) and Pentacam versus AS-OCT (Pearson correlation = 0.951, $p < 0.001$). The correlation coefficient between tono-pachymeter and the other three modalities was significantly lower than between USP, Pentacam and OCT with each other.

The ANOVA analysis (**Table 1**) showed statistically significant differences between CCT mean values from all paired instruments ($p < 0.001$ in all cases). The highest difference between pairs was found between tono-pachymeter CT-1P and USP ($-33.1 \pm 33.3 \mu\text{m}$; CI -15,2,8 to 50,9 μm ; $p < 0.001$), while the lowest difference was found between OCT and Pentacam ($-4.5 \pm 9.5 \mu\text{m}$; CI 13.3 to 22.4; $p = 0.001$) but followed too close by difference between Pentacam and USP ($-8.5 \pm 10.2 \mu\text{m}$; CI 9.4 to 26.4; $p < 0.001$) or between OCT and USP ($-13.0 \pm 6.4 \mu\text{m}$; CI 4.9 to 30.9; $p < 0.001$).

Bland-Altman analysis confirmed these results, CCT obtained by Pentacam, 3D OCT-2000 and USP pairs showed excellent agreement, with the mean difference centered close to zero, and 95% of the points were accurately located between the predicted 95% limits of agreement (**Figure 2ABC**). Conversely, tono-pachymeter CT-1P showed the lowest concordance when compared with USP, Pentacam or OCT (**Figure 2DEF**), with the higher differences (mean ± 1.96 SD). The limits of agreement 95% (LoA = mean of the difference $\pm 1.96 \times$ SD of the differences) indicates that the values on the error between the pairs of measurement have exceeded the limits of concordance. Particularly, tono-pachimetry underestimated CCT by $33.1 \mu\text{m}$ when compared with

USP, with 95% LoA ranging between 23.8 and 42.3 μm . The plot indicates that the difference between tonopachymetry and the other methods decreased significantly ($r = 0.39$; $r = 0.44$; $r = 0.43$ $p < 0.01$), showing lower CCT (proportional bias) for thinner corneas and moving to higher CCT when measuring thicker corneas (Figure 2DEF).

For a more complete reliability analysis between pairs of CCT measurements, the ICC values was calculated and can be seen in Table 1. The reliability between all pairs was statistically significant ($p < 0.001$).

Discussion

According to our findings, the average values of CCT taken with the four instruments were significantly different in healthy myopic patients. Our data demonstrated that Pentacam, AS-OCT and CT-1P tonopachymetry significantly underestimates CCT compared with the USP, considered as the gold standard, by $-8.5 \pm 10.2 \mu\text{m}$, $-13.0 \pm 6.4 \mu\text{m}$ and $-33.1 \pm 33.3 \mu\text{m}$ respectively. Several studies demonstrated that Scheimpflug-base system, as Pentacam, significantly underestimates CCT compared with USP in myopic patients before and after LASIK.^{33,34} Conversely, other authors found that Pentacam tends to overestimate CCT compared to USP after LASIK.^{35,36} Other studies have analyzed the relationship between different spectral domain AS-OCT devices from other manufactures and, in most of those papers difference between OCT and USP measurement was similar to the differences shown in this research.³⁷⁻⁴⁰ There are reports with different tonopachimetric devices, using a different operating principle (the Scheimpflug-base system), showing an underestimation of CCT when compared with USP.⁴⁰⁻⁴² However, the underestimation reported by these authors was less than difference observed in our study. Sagdik et al, also found that mean CCT was 28,4 μm thinner than USP using the CT-1P device, to the best of our knowledge the

unique study found using the same tonopachymetry system.⁴³ Moreover, we found a trend towards larger differences for thinner corneas and lower differences for thicker corneas, despite showing a moderate correlation for the difference versus mean in the Bland-Altman analysis, this is not clinically relevant.

There are many possible reasons to explain these differences, in part derived from the different operating principles of each instrument. Factors conditioning USP measurements include decentration, oblique incidence of the probe to the cornea, and the necessity for topical anesthesia, which may influence by up to 10 μm CCT measurements.¹⁴⁻¹⁵ However, apart from the much training of the operator, perpendicularity of the probe (if present) would not induce significant error as the probe is indeed quite sensitive to alignment errors. If the probe misaligns by 10° or more, the reading is not done because the “eco” is not captured by the receptor. In contrast, the indentation of the cornea by direct placement of the probe and displacement of the tear film can lead to underestimation of CCT with increased risk of corneal epithelial damage. Moreover, reliability may be influenced by variability of ultrasound speed in tissues of different hydration and dependence on examiner experience.⁴⁴⁻⁴⁵ Conversely the main advantage of the new non-contact measuring systems is that they avoid contact with the cornea, eliminating the risk of edema or epithelial damage. New AS-OCT systems include faster imaging speed (nearly 26,000 A-scans per second), higher resolution (5-6 μm of axial resolution and 20 μm of transverse resolution), and better visualization. This high-speed scanning makes ocular movements negligible during measurements, which results in a good accuracy and repeatability.^{40,46-47} The Pentacam is a Scheimpflug-base system that, non-invasively determines CCT by acquiring images on the front and back corneal surface. As mentioned above, there are controversy on CCT measurement using the Scheimpflug-base systems compared to USP.³³⁻³⁶ The tonopachymeter CT-1P uses light reflection by the front and backside of the cornea. The reflected light was brought in by the line sensor. The CCT was

measured according to the interval between the front and backside reflection images on the line sensor, so the corneal limits detection may be different than those obtained by ultrasound reflection or the Scheimpflug-base system.^{28,43} Despite the implications derived from the different algorithms that are used for CCT calculation, the differences could result too from the fixation. Pentacam, AS-OCT and CT-1P tonopachymetry have macular fixation points conditioning by the capture process, while USP is obtained by the clinician choosing where to make the measurement. These phenomena, also might be considered a measure bias in the study and explain in part the differences between non-contact devices and USP. The impact of the tear film on the measurements should also be taken into account.

Although there are various instruments utilizing different principles that can measure CCT showing significant differences, not all are equal in terms of the degree of concordance and interchangeability. Therefore, in this study we have comprehensively analyzed the relationship among the CCT values obtained using USP, Pentacam, AS-OCT and tonopachymetry systems, and we have also quantified the limit of agreement (LoA) between the CCT measurements with the pairs as plotted against their mean, using Bland–Altman plots. The mean difference between the measurements on the Bland–Altman plot is an estimate of the fixed bias in the measurements, which is the relationship of the difference in the measurements and the mean of the measurements. Our results show that CCT measurements among USP, Pentacam and AS-OCT were comparable and had significant strong positive correlations. Conversely CT-1P tonopachymetry show lower correlation and agreement when compared between USP, Pentacam or AS-OCT. Several authors demonstrated that CCT measurements performed using the Pentacam have good correlation and agreement with those performed using USP in healthy myopes.^{12,48-50} Similarly, with measures obtained with different AS-OCT devices.⁵¹⁻⁵² According to all of these results, highest agreement was accepted between Pentacam or AS-OCT and USP, hence, many authors assume that

Pentacam or modern AS-OCT can substitute USP in CCT measurement. Meanwhile, there are a few studies that suggest than Scheimpflug-base tonopachymeters were similar to Pentacam or USP in terms of agreement.⁴⁰⁻⁴² However recently Sagdik et al, found a similar agreement between CT-1P and USP which suggest that this tonopachymeter cannot be interchangeably used with USP or the other non-contact devices because of broad 95% LoA between the pairs in normal eyes.⁴³

As indicated in the methods, reliability value ranges between 0 and 1, with values closer to 1 representing stronger reliability. Historically, Pearson correlation coefficient, paired *t* test or ANOVA, and Bland-Altman plot have been used to evaluate reliability.⁵³⁻⁵⁴ However, paired *t* test or ANOVA and Bland-Altman plot are methods for analyzing agreement, and Pearson correlation coefficient is only a measure of correlation, and hence, separately they are “non-ideal” measures of reliability. However, ICC reflects both degree of correlation and agreement between measurements which indicates reliability. Thus, for a more complete analysis, ICC was assessed. ICC shows an excellent reliability between pairs except for CT-1P against the other three instruments that were found moderate. The relationship between values obtained by AS-OCT compared with the USP showed the highest ICC, while matching values obtained with CT-1P tonopachymetry and USP had the lowest ICC (**Table 2**). These relationships, coupled with the differences, confirm that the CCT measurements obtained by CT-1P tonopachymetry are not interchangeable with those obtained by USP. On the contrary, the lower differences between AS-OCT or Pentacam when compared with USP and their high ICC suggest the possibility of interchanging their values.

There are some limitations to this study. We excluded subjects with severe myopia, astigmatism of more than 1.75 D, irregular astigmatism, refractive surgery, and ocular pathologies, for which any bias between instruments could have clinical implications, and thus, our findings may hold true only for subjects with similar refraction

characteristics. Furthermore, the sample size of this study was relatively small, future studies will need to include larger populations, with different ocular conditions.

In conclusion, our data suggest that the clinician should be aware of significant differences of CCT values when measuring with different devices. Furthermore, in clinical settings where CCT values are critical, we suggest that the CCT results of the CT-1P versus USP and the CT-1P versus Pentacam or CT-1P versus AS-OCT should not be used interchangeably. Given mean differences and range variations in CCT measurements between devices, AS-OCT, Scheimpflug-based system and USP could be interchangeable to measure CCT in healthy subjects. However, in clinical practice, these three modalities should be tested in different pathologic conditions. Although CCT values measured with Pentacam, AS-OCT and USP are closely similar, clinicians should keep in mind that these methods are not simply interchangeable.

References

1. Brandt JD. Corneal thickness in glaucoma screening, diagnosis, and management. *Curr Opin Ophthalmol* 2004; 15: 85-9.
2. Schweitzer C, Roberts CJ, Mahmoud AM, Colin J, Maurice-Tison S, Kerautret J. Screening of forme fruste keratoconus with the ocular response analyzer. *Invest Ophthalmol Vis Sci* 2010; 51: 2403-2410.
3. Hori-Komai Y, Toda I, Asano-Kato N, Tsubota K. Reasons for not performing refractive surgery. *J Cataract Refract Surg* 2002; 28: 795-7.
4. Grewal DS, Brar GS, Grewal SP. Assessment of central corneal thickness in normal, keratoconus, and post-laser in situ keratomileusis eyes using Scheimpflug imaging, spectral domain optical coherence tomography, and ultrasound pachymetry. *Journal of Cataract and Refractive Surgery* 2010;36:954-64.

5. Gonzalez-Meijome JM, Gonzalez-Perez J, Cervino A, Yebra-Pimentel E, Parafita MA. Changes in corneal structure with continuous wear of high-Dk soft contact lenses: a pilot study. *Optom Vis Sci* 2003;80:440-446.
6. Gonzalez-Perez J, González-Meijome JM, Jalbert I, Sweeney DF, Erickson P. Corneal epithelial thinning profile induced by long-term wear of hydrogel lenses. *Cornea* 2003;22:304-307.
7. Bayraktar, S. and Bayraktar, Z. Central corneal thickness and intraocular pressure relationship in eyes with and without previous LASIK: comparison of Goldmann applanation tonometer with pneumatonometer. *Eur J Ophthalmol* 2005;15:81-88.
8. Ciolino JB, Khachikian SS, Belin MW. Comparison of corneal thickness measurements by ultrasound and Scheimpflug photography in eyes that have undergone laser in situ keratomileusis. *Am J Ophthalmol* 2008;145:75–80.
9. Gordon MO, Beiser JA, Brandt JD. The Ocular hypertension treatment study: baseline factors that predict the onset of primary open-angle glaucoma. *Arch Ophthalmol* 2002;120:714- 20.
10. Wang SY, Melles R, Lin SC. The impact of central corneal thickness on the risk of glaucoma in a large multiethnic population. *J Glaucoma* 2014;23:606-612.
11. Doughty MJ, Zaman ML. Human corneal thickness and its impact on intraocular pressure measures: a review and meta-analysis approach. *Surv Ophthalmol* 2000;44:367-408.
12. González-Pérez J, González-Méijome JM, Rodríguez Ares MT, Parafita MA. Central corneal thickness measured with three optical devices and ultrasound pachometry. *Eye Contact Lens* 2011;37:66–70.
13. Williams R, Fink BA, King-Smith PE, Mitchell GL. Central corneal thickness measurements: using an ultrasonic instrument and 4 optical instruments. *Cornea* 2011;30:1238-43.

14. Asensio I, Rahhal SM, Alonso L, Palanca-Sanfrancisco JM, Sanchis-Gimeno JA. Corneal thickness values before and after oxybuprocaine 0.4% eye drops. *Cornea* 2003;22:527-532.
15. Sedaghat MR, Daneshvar R, Kargozar A, Derakhshan A, Daraei M. Comparison of central corneal thickness measurement using ultrasonic pachymetry, rotating Scheimpflug camera, and scanning-slit topography. *Am J Ophthalmol* 2010;150:780-789.
16. Huang D, Swanson EA, Lin CP, Schuman JS, Stinson WG, Chang W, et al. Optical coherence tomography. *Science* 1991;254:1178–1181.
17. Chen TC, Cense B, Pierce MC, Nassif N, Park BH, Yun SH, et al. Spectral-domain optical coherence tomography: ultra high-speed, ultra high-resolution ophthalmic imaging. *Arch Ophthalmol* 2005;123:1715–1720.
18. González-García AO, Vizzeri G, Bowd C, Medeiros FA, Zangwill LM, Weinreb RN. Reproducibility of RTVue retinal nerve fiber layer thickness and optic disc measurements and agreement with Stratus optical coherence tomography measurements. *Am J Ophthalmol* 2009;147:1067–1074.
19. Kashani AH, Chen CL, Gahm JK, Zheng F, Richter GM, Rosenfeld PJ, et al. Optical coherence tomography angiography: A comprehensive review of current methods and clinical applications. *Prog Retin Eye Res* 2017;60:66-100.
20. Leitgeb R, Hitzenberger CK, Fercher AF. Performance of Fourier-domain vs. time-domain optical coherence tomography. *Opt Express* 2003;11:889–894.
21. Sakata LM, Lavanya R, Friedman DS, Aung HT, Gao H, Kumar RS, et al. Comparison of gonioscopy and anterior segment optical coherence tomography in detecting angle closure in different quadrants of the anterior chamber angle. *Ophthalmology* 2008;115:769–774.
22. Doors M, Tahzib NG, Eggink FA, Berendschot TT, Webers CA, Nuijts RM. Use of anterior segment optical coherence tomography to study corneal changes after collagen cross-linking. *Am J Ophthalmol* 2009;148:844–851.

23. Chen Q, Wang J, Shen M, Cai C, Li J, Cui L, et al. Lower volumes of tear menisci in contact lens wearers with dry eye symptoms. *Invest Ophthalmol Vis Sci* 2009;50:3159–3163.
24. Ang M, Cai Y, Tan AC. Swept Source Optical Coherence Tomography Angiography for Contact Lens-Related Corneal Vascularization. *J Ophthalmol* 2016;2016:1-3.
25. Ramesh PV, Jha KN, Srikanth K. Comparison of Central Corneal Thickness using Anterior Segment Optical Coherence Tomography Versus Ultrasound Pachymetry. *J Clin Diagn Res* 2017;11:NC08-NC11.
26. Huang J, Ding X, Savini G, Pan C, Feng Y, Cheng D, et al. A comparison between scheinpflug imaging and optical coherence tomography in measuring corneal thickness. *Ophthalmology* 2013;120:1951–1958.
27. Al-Mezaine HS, Al-Amro SA, Kangave D, Sadaawy A, Wehaib TA, Al-Obeidan S. Comparison between central corneal thickness measurements by oculus pentacam and ultrasonic pachymetry. *Int Ophthalmol*. 2008;28:333-8.
28. Barkana Y, Gerber Y, Elbaz U, Schwartz S, Ken-Dror G, Avni I, et al. Central corneal thickness measurement with the Pentacam Scheimpflug system, optical low-coherence reflectometry pachymeter, and ultrasound pachymetry. *J Cataract Refract Surg* 2005;31:1729–1735.
29. Fujimura F, Kamiya K, Fujiwara K, Shoji N, Shimizu K. Repeatability and reproducibility of measurements using a NT-530P noncontact tono/pachymeter and correlation of central corneal thickness with intraocular pressure. *Biomed Res Int* 2013;2013:1-5.
30. Du Toit R, Vega JA, Fonn D, Simpson T. Diurnal variation of corneal sensitivity and thickness. *Cornea* 2003;22:205–209.
31. Shrout PE, Fleiss JL. Intraclass correlations: uses in assessing rater reliability. *Psychol Bull* 1979;86:420-8.
32. Bland JM, Altman DG. Statistical methods for assessing agreement between two methods of clinical measurement. *Lancet* 1986;1:307–310.

33. Ho T, Cheng AC, Rao SK, Lau S, Leung CK, Lam DS. Central corneal thickness measurements using Orbscan II, Visante, ultrasound, and Pentacam pachymetry after laser in situ keratomileusis for myopia. *J Cataract Refract Surg* 2007;33:1177–82.
34. Hashemi H, Mehravaran S. Central corneal thickness measurement with Pentacam, Orbscan II, and ultrasound devices before and after laser refractive surgery for myopia. *J Cataract Refract Surg* 2007;33:1701–7.
35. Al-Mezaine HS, Al-Amro SA, Kangave D, Al-Obeidan S, Al-Jubair KM. Comparison of central corneal thickness measurements using Pentacam and ultrasonic pachymetry in post-LASIK eyes for myopia. *Eur J Ophthal* 2010;20:852–7.
36. Tai LY, Khaw KW, Ng CM, Subrayan V. Central corneal thickness measurements with different imaging devices and ultrasound pachymetry. *Cornea* 2013;32:766–1.
37. Rao HL, Kumar AU, Kumar A, Chary S, Senthil S, Vaddavalli PK, et al. Evaluation of central corneal thickness measurement with RTVue spectral domain optical coherence tomography in normal subjects. *Cornea* 2011;30:121-126.
38. Kanellopoulos AJ, Asimellis G. Comparison of high-resolution Scheimpflug and high-frequency ultrasound biomicroscopy to anterior-segment OCT corneal thickness measurements. *Clin Ophthalmol* 2013;7:2239-2247.
39. Northey LC, Gifford P, Boneham GC. Comparison of Topcon optical coherence tomography and ultrasound pachymetry. *Optom Vis Sci* 2012;89:1708-1714.
40. Lee YG, Kim JH, Kim NR, Kim CY, Lee ES. Comparison between Tonopachy and other tonometric and pachymetric devices. *Optom Vis Sci* 2011;88:843-9.
41. Lomoriello DS, Lombardo M, Tranchina L, Oddone F, Serrao S, Ducoli P. Repeatability of intra-ocular pressure and central corneal thickness measurements provided by a non-contact method of tonometry and pachymetry. *Graefe's Arch Clin Exp Ophthalmol* 2011;249:429-34.

42. Garcia-Resua C, Blanco A, Miñones M, Yebra-Pimentel E, Jesus Giraldez M. Accuracy and repeatability of a new tono-pachymeter for measuring central corneal thickness. *Eye Contact Lens* 2012;38:158-63.
43. Sagdik HM, Aktas S, Tetikoglu M, Ozcura F. Comparison of ultrasonic pachymetry, with a new optical biometry and tono-pachymetry. *Medicine Science* 2017;6:22- 5.
44. Gonzalez- Meijome JM, Cervino A, Yebra-Pimentel E & Parafita MA. Central and peripheral corneal thickness measurement with Orbscan II and topographical ultrasound pachymetry. *J Cataract Refract Surg* 2003;29: 125–132.
45. Nemeth G, Tsorbatzoglou A, Kertesz K, Vajas A, Berta A & Modis L Jr. Comparison of central corneal thickness measurements with a new optical device and a standard ultrasonic pachymeter. *J Cataract Refract Surg* 2006;32: 460–463.
46. Lackner B, Schmidinger G, Pieh S, Funovics MA, Skorpik C. Repeatability and reproducibility of central corneal thickness measurement with Pentacam, Orbscan, and ultrasound. *Optom Vis Sci* 2005;82:892-899.
47. Bayhan HA, Aslan Bayhan S, Can I. Comparison of central corneal thickness measurements with three new optical devices and a standard ultrasonic pachymeter. *Int J Ophthalmol* 2014;7:302-308.
48. Ciolino JB, Khachikian SS, Belin MW. Comparison of corneal thickness measurements by ultrasound and Scheimpflug photography in eyes that have undergone laser in situ keratomileusis. *Am J Ophthalmol* 2008;145:75–80.
49. Sedaghat MR, Daneshvar R, Kargozar A, Derakhshan A, Daraei M. Comparison of central corneal thickness measurement using ultrasonic pachymetry, rotating Scheimpflug camera, and scanning-slit topography. *Am J Ophthalmol* 2010;150:780–9.
50. Sadoughi MM, Einollahi B, Einollahi N, Rezaei J, Roshandel D, Feizi S. Measurement of Central Corneal Thickness Using Ultrasound Pachymetry and Orbscan II in Normal Eyes. *J Ophthalmic Vis Res* 2015;10:4–9.

51. Calvo-Sanz JA, Ruiz-Alcocer J, Sánchez-Tena MA. Accuracy of Cirrus HD-OCT and Topcon SP-3000P for measuring central corneal thickness. *J Optom* 2017;18: S1888-4296(17)30002-X. doi: 10.1016/j.optom.
52. Ramesh PV, Jha KN, Srikanth K. Comparison of Central Corneal Thickness using Anterior Segment Optical Coherence Tomography Versus Ultrasound Pachymetry. *J Clin Diagn Res* 2017;11:NC08-NC11.
53. Brown BW, Jr., Lucero RJ, Foss AB. A situation where the Pearson correlation coefficient leads to erroneous assessment of reliability. *J Clin Psychol* 1962;18:95–97.
54. Landis JR, Koch GG. The measurement of observer agreement for categorical data. *Biometrics* 1977;33:159-174.

Accepted Manuscript

Table 1. Comparisons among pairs of instruments, average difference, upper and lower 95% confidence limits, statistical significance and Pearson correlation coefficient. Values are in microns. Calculation in SPSS using multivariate analysis of variance (ANOVA) in the general lineal model.

Pairwise Comparison	Mean Diff.	95% Confidence Interval	Sig (p-value)*	Correlation Pearson
USP vs Pentacam	8.5±10.2	9.4 to 26.4	<0.001	0.946
USP vs 3D OCT	13.0±8.4	4.9 to 30.9	<0.001	0.979
USP vs CT-1P	33.1±33.3	-15.2 to 50.9	<0.001	0.640
Pentacam vs 3D OCT	4.5±9.5	13.3 to 22.4	0.001	0.951
Pentacam vs CT-1P	24.6±30.8	-6.7 to 42.5	<0.001	0.700
3D OCT vs CT-1P	20.0±31.3	-2.1 to 37.9	<0.001	0.687

*Multivariate ANOVA using Bonferroni adjustment for multiple comparisons. USP: Ultrasound pachymetry; ANOVA: Analysis of variance.

Table 2. Results of intraclass correlation coefficient (ICC), upper and lower 95% confidence limits and statistical significance. Calculation in SPSS using two-way random model.

Pairs-Parameter	ICC	95% Confidence Interval	Sig (p-value)
USP vs Pentacam	0.946	0.807 to 0.968	< 0.001
USP vs 3D OCT	0.978	0.863 to 0.987	< 0.001
USP vs CT-1P	0.608	0.303 to 0.759	< 0.001
Pentacam vs 3D OCT	0.951	0.839 to 0.972	< 0.001
Pentacam vs CT-1P	0.660	0.375 to 0.790	< 0.001
3D OCT vs CT-1P	0.648	0.347 to 0.781	< 0.001

Figure 1 Scattered plot analysis of CCT showing a significant positive strong correlation between CCT measured by: A) USP and Pentacam (slope=0.946, $R^2=0.895$); B) USP and 3D OCT-2000 (slope=0.979, $R^2=0.957$); C) Pentacam and 3D OCT-2000 (slope=0.951, $R^2=0.905$); D) USP (slope=0.640, $R^2=0.409$); E) Pentacam (slope=0.700, $R^2=0.490$); F) 3D OCT-2000 (slope=0.687, $R^2=0.471$).


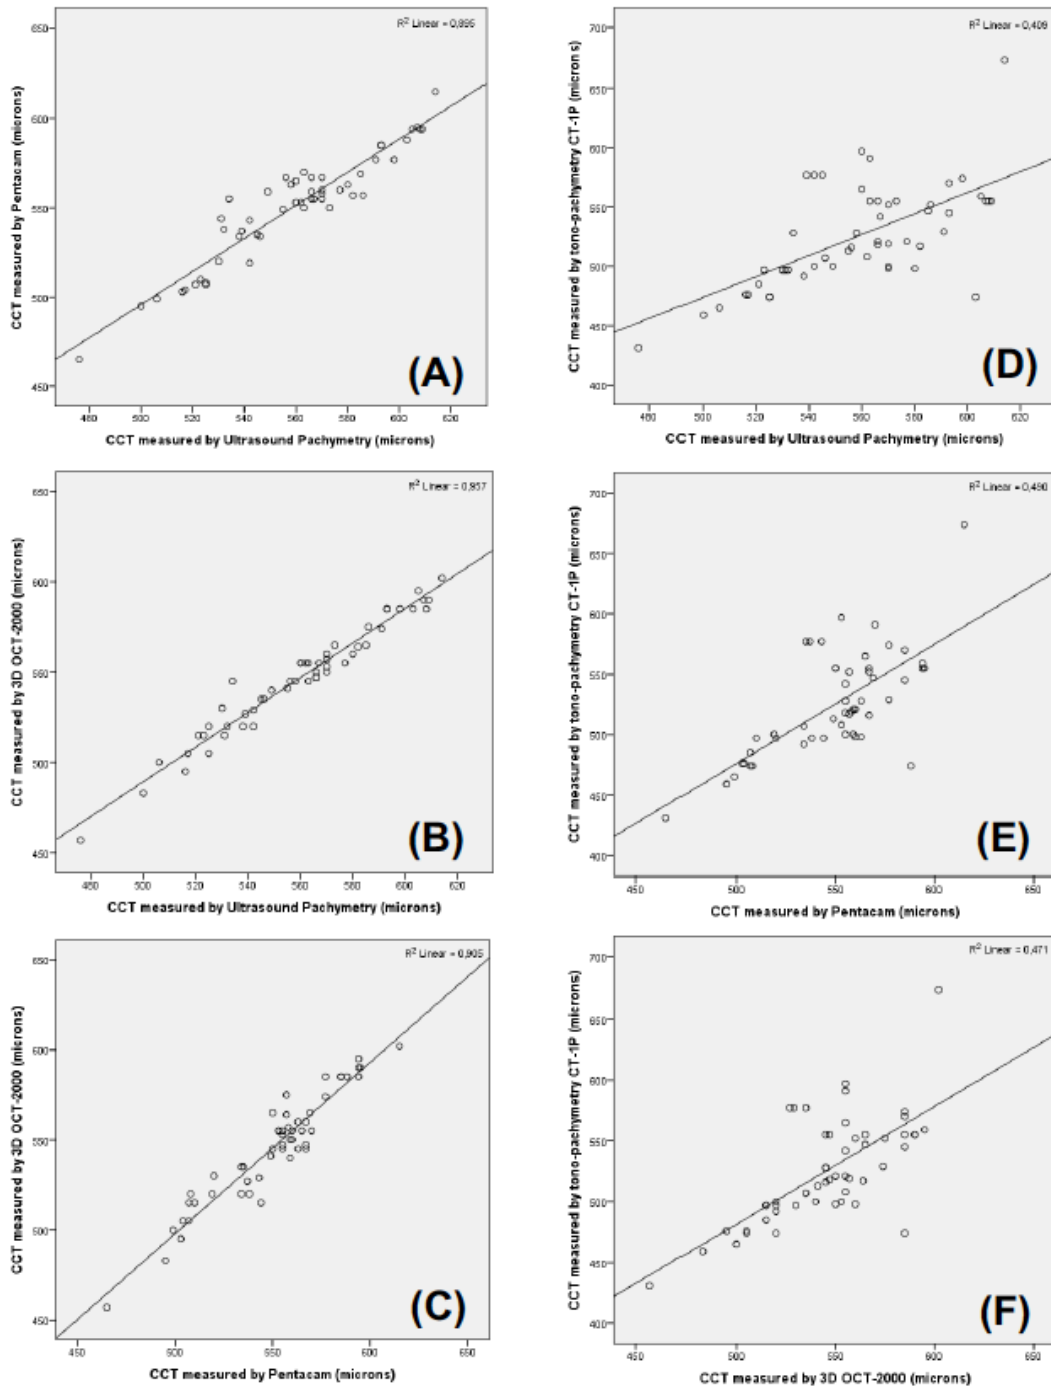


Figure 2 Bland-Altman analysis. Mean difference (solid line) and 95% limits of agreement-LoA (dashed line) for CCT. Mean differences were: A) 8.5 μm with 95% LoA from -11.4 to 28.4 μm for the USP/Pentacam pair; B) 13.0 μm with 95% LoA from 0.4 to 25.6 μm for the USP/AS-OCT pair; C) 4.5 μm with 95% LoA from -14.1 to 23.2 μm for the Pentacam/AS-OCT pair; D) 33.1 μm with 95% LoA from -32.2 to 98.3 μm for the USP/CT-1P pair; E) 20.0 μm with 95% LoA from -

41.4 to 81.5 μm for the AS-OCT/ CT-1P pair; F) 24.6 μm with 95% LoA from -35.7 to 84.9 μm for the Pentacam/ CT-1P pair.

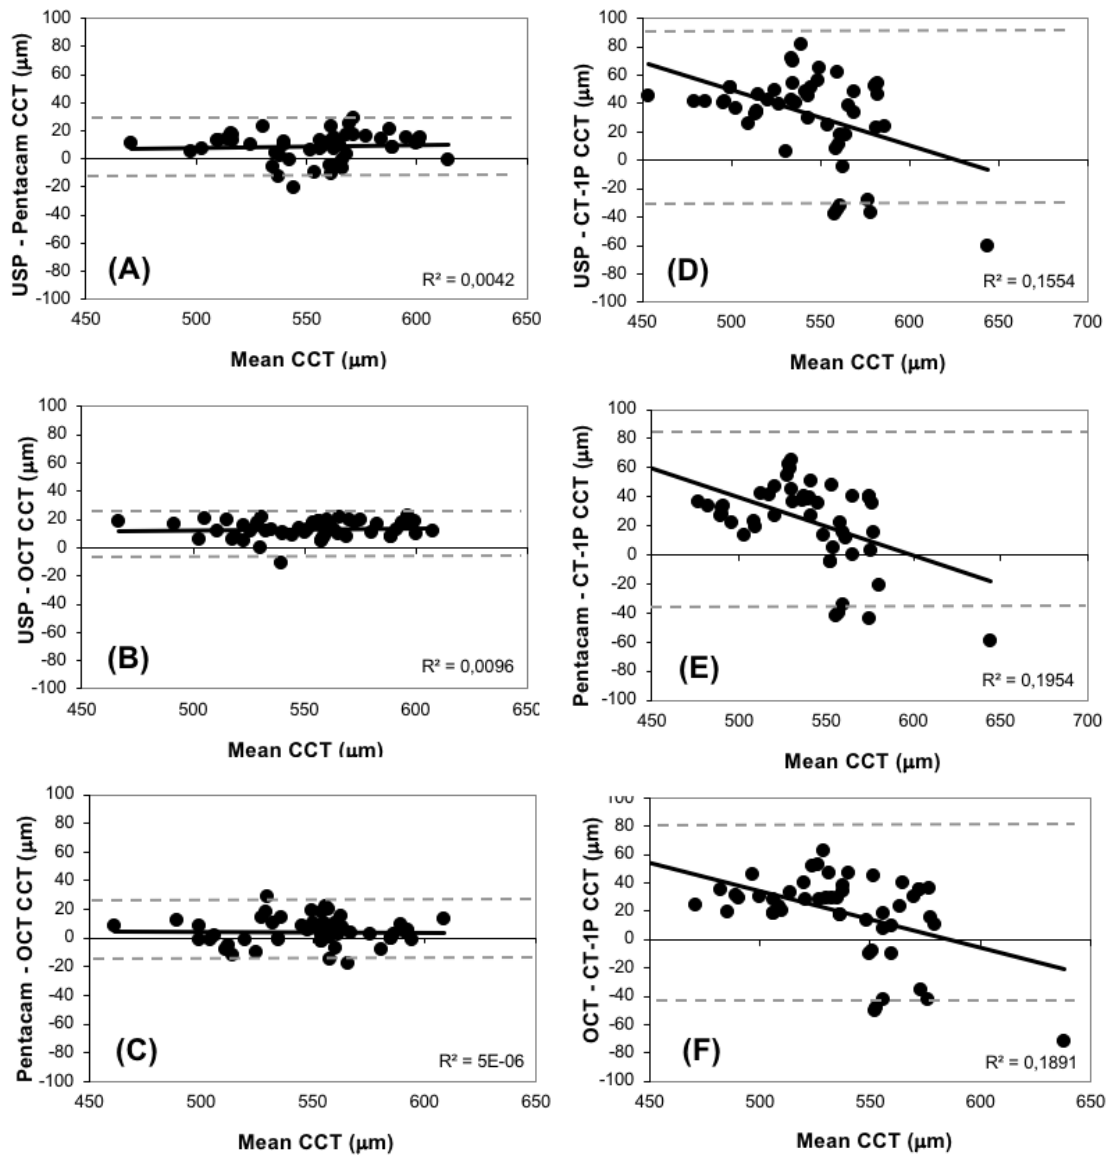

ACC