

APPLICATION OF CYCLIC VOLTAMMETRIC TECHNIQUE ON DYE CONCENTRATION CONTROL IN AQUEOUS SOLUTIONS

M. de Fátima Esteves^{1*}, M.T.Pessoa de Amorim¹, C. Cornel²

¹*Departamento de Engenharia Têxtil, Escola de Engenharia, Universidade do Minho, P-4800
Guimarães*

²*Laboratoire de Chimie et Environnement, U.F.R. Sciences, Université d'Angers,
F-49045 Angers Cedex*

Abstract

This communication follows a previous work concerning indirect electrochemical reduction of dyes [1] and its application on dyeing control with sulphur dyes.

The study concerns the cathodic peak intensity variation with sulphur dye C.I. Leuco Sulphur Black 1 (Black Diresul RDT liq.) concentration, in the presence of a mediator, iron/triethanolamine (Fe^{III}/TEA), in alkaline media.

Key Words: Mediator redox couple, reversible electron-transfer, cathodic peak intensity, dye concentration

1.Introduction

Earlier cyclic voltammetric studies with glass carbon electrodes [1] showed a linear correlation between cathodic peak intensity and dye concentration. Experimental conditions, namely, pH value and mediator electron-transfer potential [2] are on the limit of glass carbon application as working electrode material [3,4]. The observed electrode behaviour changes made the reduction peak detection more difficult [5].

In consequence of these facts, other materials were studied in order to be used as working electrodes. The results showed that copper allows a higher electron-transfer reversibility, as well as their reproducibility [5].

2.Experimental

Apparatus

A three-electrode cell was used: copper working electrode ($\text{\O} 4$ mm, Radiometer) platinum counter electrode (Ingold), saturated calomel reference electrode, SCE (Ingold). This cell was connected to a HI-TEK PPR 1 wave generator and a HI-TEK DT 2101 potentiostat, as previous scheme [1,5]. A data acquisition program (Picolog) was incorporated in a connected computer.

Materials and Solutions

The mediator system was used in an earlier tested composition [5]. The cyclic voltammetric experiments were obtained at $25\pm 0,1^\circ\text{C}$, with a $[-800, -1200$ mV] potential sweep and a 20 mVs⁻¹ scanning rate.

3.Results and Discussion

Figure 1 represents the cyclic voltammogram for the mediator system Fe^{III}/TEA.

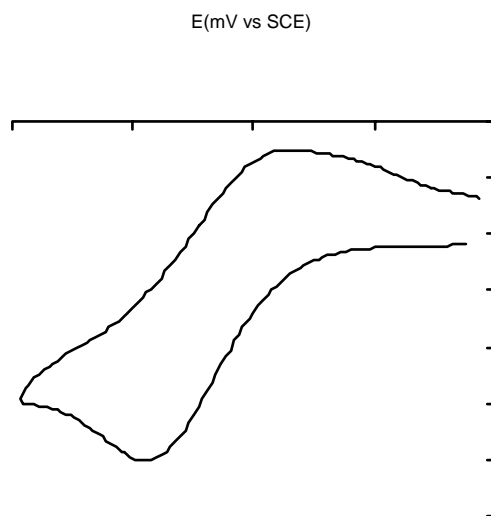


Fig.1. Cyclic voltammogram for the mediator system
 $5 \text{ gL}^{-1}\text{Fe}_2(\text{SO}_4)_3 \cdot x \text{ H}_2\text{O}$; $4 \text{ gL}^{-1}\text{TEA}$; $8 \text{ gL}^{-1}\text{NaOH}$

In figure 2, mediator system voltammograms in the presence of dye are presented.

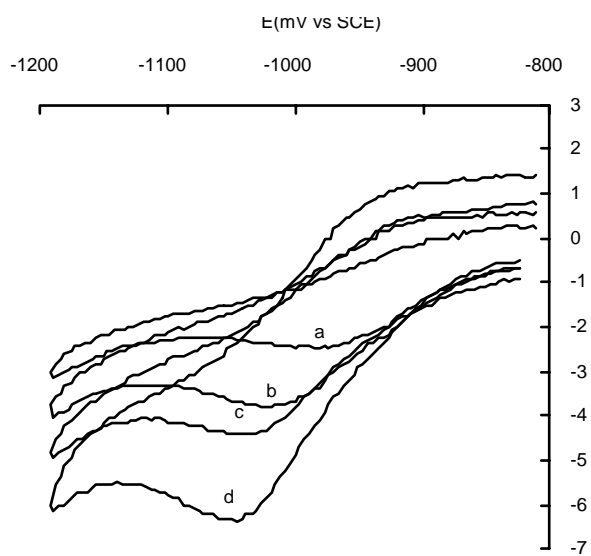


Fig.2. Cyclic voltammograms for the mediator system in the presence of dye
 $0.8^a, 1.6^b, 2.4^c, 3.2^d \text{ gL}^{-1}$

Figure 1 analysis shows that, in these experimental conditions, Fe^{3+} -TEA/ Fe^{2+} -TEA electron-transfer occurs reversibly, at a potential near to -1092 mV vs ESC [2].

In the presence of dye, figure 2, the anodic peak disappearance is detected, which agrees with a non electrodic mediator oxidation, due to the reduction of the dye into the solution[2]. An increase in cathodic peak intensity is also observed. This variation can be explained by an increase in mediator system action with dye concentration [2].

Figure 3 represents the relation between cathodic peak intensity and dye concentration, in the considered experimental conditions.

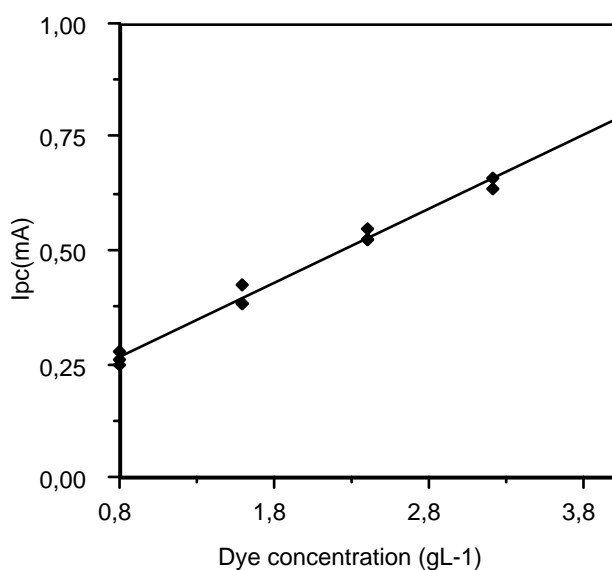


Fig.3. Cathodic peak intensity and dye concentration relation

With least-squares method a correlation was established between cathodic peak intensity and dye concentration, with a coefficient of 0,990.

4. Conclusions

Considering all the presented experimental results we can conclude that, in the case of the studied sulphur dye, C.I. Leuco Sulphur Black 1 (Black Diresul RDT liq.) is possible to establish, in aqueous solution, a linear correlation between cathodic peak intensity and its concentration.

This relation seems to be independent of electrode material [2], being this one appropriate to pH and potential conditions.

These experimental results were obtained for aqueous solutions of the dye. The application of this technique to dyeing baths control will require a study with more complex solutions, of composition similar to those founded in dyeing processes to check the interference of the other chemicals products.

5. References

- 1-F. Esteves, M.T. Amorim, C. Comel, *4ª Conferência Nacional Sobre a Qualidade do Ambiente*, Lisboa (1994)
- 2-T. Bechtold, E. Burtscher, D. Gmeiner, O. Bobleter, *J. Electroanal. Chem.*, 306 (1991) 171.
- 3-EG&G Princeton Applied Research - Technical informations - Micro-Cell Accessories (1995) E4
- 4-D.T. Sawyer, A. Sobkowiak, J.L. Roberts, jr., *Electrochemistry for Chemists*, John Wiley and Sons (1995) 208
- 5-M. Fátima Esteves, M.T. Amorim, *Portugaliae Electroquímica Acta*, 14 (1996) 261-265